

The WalkAide® Functional Electrical Stimulation System—A Novel Therapeutic Approach For Foot Drop in Central Nervous System Disorders

Michelle H Cameron, MD, PT

Neurologist, Multiple Sclerosis Center of Excellence West, Portland Veterans Affairs Medical Center, and
Assistant Professor, Department of Neurology, Multiple Sclerosis Center of Oregon, Oregon Health and Science University

Abstract

Foot drop is the inability to voluntarily dorsiflex the ankle during the swing phase of gait. Foot drop decreases gait quality, limits mobility, increases fall risk, and greatly increases energy expenditure during walking. Traditionally, foot drop is treated with passive dorsiflexion support by an ankle foot orthosis (AFO) but today, functional electrical stimulation (FES) devices are available to promote comfortable, effective active dorsiflexion during gait for patients with central nervous system (CNS) causes of foot drop. The WalkAide® FES System's unique control system, with tilt sensors to trigger electrical stimulation during swing phase, can help normalize gait and thus optimize safety, cosmesis, and energy efficiency in people with stroke, multiple sclerosis, cerebral palsy, and a wide range of other CNS disorders.

Keywords

Brain injuries, cerebral palsy, electric stimulation therapy, gait, multiple sclerosis, stroke, walking

Disclosure: Michelle H Cameron, MD, PT, has received compensation for consulting from Teva Neurosciences, Mettler Electronics, Chattanooga Group, and Innovative Neurotronics.

Received: September 20, 2010 **Accepted:** November 12, 2010 **Citation:** *US Neurology*, 2010;6(2):112-4 DOI: 10.17925/USN.2010.06.02.112

Correspondence: Michelle H Cameron, MD, PT, Department of Neurology, 3181 SW Sam Jackson Park Road, L226, Portland, OR 97239-3098. E: cameromi@ohsu.edu

Support: The publication of this article was funded by Innovative Neurotronics, Inc. The views and opinions expressed are those of the author and not necessarily those of Innovative Neurotronics, Inc.

Foot drop is the inability to voluntarily dorsiflex the ankle and thereby lift the foot during the swing phase of gait. The condition is characterized by dragging the foot, which causes tripping or a steppage gait where the person raises their knee high during swing phase to avoid tripping over the hanging down foot and then, at the beginning of stance phase, the foot slaps the floor. Gait changes caused by foot drop decrease gait safety and efficiency, limit mobility, increase the risk for falls, and greatly increase energy expenditure during walking.^{1,2}

Causes of Foot Drop

Foot drop is usually caused by damage to areas of the nervous system that control ankle dorsiflexion. Foot drop may be caused by central or peripheral nerve dysfunction and is common in patients with a wide variety of neurologic diagnoses including stroke, multiple sclerosis (MS), traumatic brain injury (TBI), spinal cord injury (SCI), cerebral palsy (CP), and peripheral neuropathy.

Treatment of Foot Drop


Traditionally, foot drop of all etiologies is treated with bracing using an ankle foot orthosis (AFO) (see *Figure 1A*). An AFO is a device, usually made of plastic, which wraps under the foot and behind the calf to passively assist ankle dorsiflexion. AFOs are simple devices that are

widely available at relatively low cost, but they have a number of disadvantages and limitations. The passive dorsiflexion assistance they provide does not promote active use of remaining or recovering dorsiflexion function and also limits ankle range of motion. In addition, AFOs can be uncomfortable, bulky, and, if poorly fitted, produce areas of pressure and tissue breakdown. Many patients find AFOs so uncomfortable or unsightly that they do not use them. Research has therefore focused on developing alternative ways to treat foot drop. One of the most effective treatments for foot drop is functional electrical stimulation (FES, see *Figure 1B*).²⁻⁵

Who Can Use the WalkAide® Functional Electrical Stimulation System for Foot Drop?

FES is a new approach to treating foot drop. FES uses a low-level electrical current to stimulate peripheral motor nerves to produce active muscle contractions that promote functional movement. FES for foot drop involves stimulating the peroneal nerve to produce active dorsiflexion during the swing phase of gait. FES can be used to treat foot drop when the CNS is damaged and the peripheral nerves, neuromuscular junction, and muscles are intact. Therefore, FES is particularly effective for treating foot drop caused by CNS disorders such as stroke,⁶⁻⁸ MS,^{3,9-11} TBI,¹² incomplete SCI,¹³⁻¹⁵ and CP^{16,17} as well as other, less common CNS disorders.

Figure 1: Options for Treatment of Foot Drop

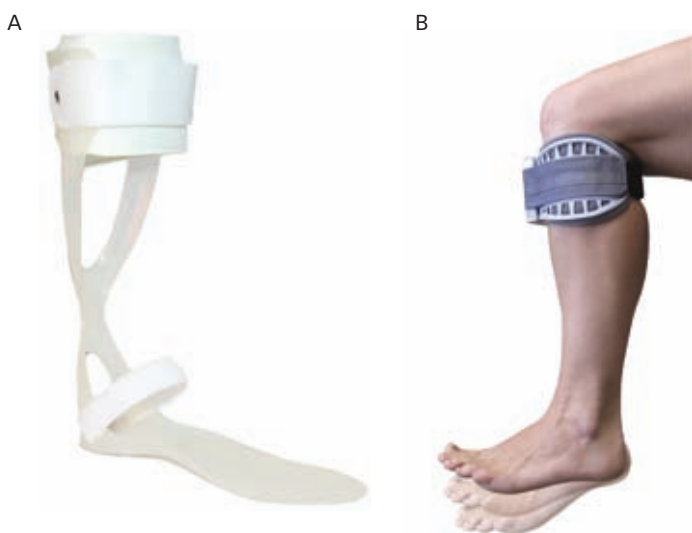

A: A traditional ankle foot orthosis; B: The WalkAide Functional Electrical Stimulation System.

How the WalkAide Functional Electrical Stimulation System Treats Foot Drop

The WalkAide® FES System is a non-invasive, self-contained device designed specifically to provide comfortable and effective transcutaneous stimulation to the peroneal nerve to improve dorsiflexion during the swing phase of gait. The WalkAide FES System is contained in a cuff worn around the proximal leg just below the knee (see Figure 1B). The device includes tilt sensors, with accelerometers and inclinometers to measure the speed and position of the lower leg to trigger stimulation, and a pulse generator and self-adhesive electrodes to deliver the electrical current. The entire device is powered by a single AA battery. With the WalkAide, low intensity pulses of electrical current, of sufficient duration and amplitude to produce action potentials in peripheral nerves, are delivered from the generator to transcutaneous self-adhesive electrodes placed over the common peroneal nerve near the fibular head (see Figure 2). The stimulated action potentials are transmitted orthodromically to the superficial and deep peroneal nerves, and thence to the neuromuscular junctions of the muscles of the lateral and anterior compartment of the leg. This causes acetylcholine release at the neuromuscular junctions and muscle contractions to produce active ankle dorsiflexion. The tilt sensors trigger the electrical current pulses to start just as the patient enters the swing phase of gait and to end when swing ends. This produces dorsiflexion throughout swing phase, minimizing or entirely eliminating foot drop and normalizing the gait pattern.

Features and Advantages of the WalkAide Functional Electrical Stimulation System

FES has a number of advantages over an AFO for treatment of foot drop. (see Table 1) The active contraction produced by FES can help prevent the muscle atrophy and range of motion loss associated with passive support offered by an AFO. In addition, the active muscle contractions and joint motion stimulate muscle spindles, Golgi tendon organs, and joint proprioceptors, increasing sensory awareness and input to the CNS. This sensory input improves motor output, including the quality and control of movement patterns, the degree of reflex activity, and the

Figure 2: The WalkAide System Delivering Electrical Stimulation to the Common Peroneal Nerve and Produces Timed Contraction of the Dorsiflexor Muscles



Figure 3: The WalkAide System Has the Unit and Cuff in a Single Component and Can Be Used Without Shoes

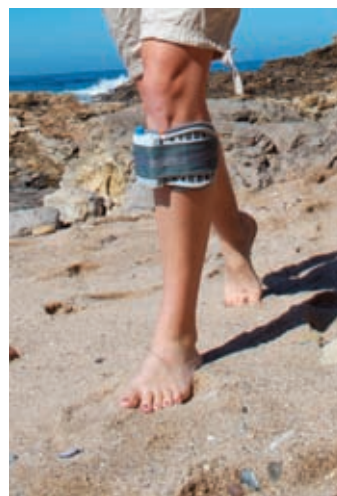


Table 1: Comparison of Benefits of Funtional Electrical Stimulation and Ankle Foot Orthosis for Foot Drop

	FES	AFO
Reduces foot drop	Yes	Yes
Improves gait mechanics	Yes	Yes
Prevents loss of passive ROM	Yes	Yes
Prevents loss of active ROM	Yes	No
Active muscle contraction	Yes	No
Slows muscle atrophy	Yes	No
Increases input to muscle spindles, GTOs, proprioceptors	Yes	No
Promotes motor learning	Yes	No
Promotes neuroplastic changes	Yes	No

AFO = ankle foot orthosis; FES = functional electrical stimulation; GTO = Golgi tendon organ; ROM = range of motion.

balance of muscle tone. The repetitive active movement stimulated by FES-facilitated gait also contributes to motor learning and neuroplastic changes in the CNS.¹⁸ By establishing and promoting active motion in patients with foot drop, FES fosters long-term improvements in motor control, balance of muscle activation, and quality and efficiency of gait. Unique features of the WalkAide FES System make it particularly well suited to the treatment of foot drop. The WalkAide is the only device on the market that uses tilt sensors to detect the angular velocity of the leg during gait and to use this information to determine when to trigger stimulation, and thus muscle contraction, during the gait cycle.¹⁹ Most other devices use a heel-sensor-triggered switch to detect the beginning and end of swing phase. Since heel switch devices stimulate whenever the heel is off the ground, stimulation may occur when the heel, but not the toes, are raised. This can promote inefficient walking patterns including steppage gait and stiff legged walking with hip circumduction and vaulting. By triggering stimulation specifically in response to leg movement in the sagittal plane, the WalkAide stimulates dorsiflexion when the patient swings their leg straight through in the sagittal plane. This unique tilt sensor triggered stimulation promotes normal gait not only by stimulating optimal timing of ankle dorsiflexion during gait but also by helping the patient decrease compensatory motions and improve voluntary motor control at the hip and knee. All of these features contribute to the WalkAide allowing the person with foot drop to walk faster, more safely, and with reduced energy consumption.^{1,15,18-21}

The WalkAide FES System can also be precisely tailored to each individual's gait pattern and can adapt to a range of patient-initiated

changes in gait. It alters the timing of the stimulation if walking speed or direction, or step length, change. It also adapts to changes produced by different gait tasks, such as walking up or down stairs or inclines or walking on rough terrain. Having a tilt sensor on the leg rather than a heel switch also allows the patient to use the WalkAide with a wide variety of footwear, or even to walk barefoot (see *Figure 3*). All of these features give the patient improved function during a wide range of activities of daily living and improve quality of life. The unique design and construction of the WalkAide System further contribute to its utility. The entire device is essentially contained in one component. The unit attaches to a lightweight cuff strapped around the leg that can be accurately placed and fully operated with one hand. The cuff is fully washable and the device is powered by a single AA battery that lasts for up to one month of use. The WalkAide System offers you and your patients the latest advance in the treatment of foot drop. It is the most physiologic and effective approach for optimizing gait mechanics and efficiency in patients with foot drop, allowing them to walk quickly, efficiently, and safely in the widest range of conditions. ■



Michelle H Cameron, MD, PT, is a Neurologist at the Multiple Sclerosis Center of Excellence West at the Portland Veterans Affairs Medical Center and at the Multiple Sclerosis Center of Oregon at Oregon Health and Science University (OHSU), and an Assistant Professor in the Department of Neurology at OHSU. She researches balance and falls in multiple sclerosis and has authored text books, peer-reviewed articles, and abstracts.

- Stein RB, et al., Long-term therapeutic and orthotic effects of a foot drop stimulator on walking performance in progressive and non-progressive neurological disorders, *Neurorehabil Neural Repair*, 2010;24:152-67.
- Sheffler LR, et al., Peroneal nerve stimulation versus an ankle foot orthosis for correction of footdrop in stroke: Impact on functional ambulation, *Neurorehabil Neural Repair*, 2006;20:355-60.
- Sheffler LR, et al., Spatiotemporal and kinematic effect of peroneal nerve stimulation versus an ankle-foot orthosis in patients with multiple sclerosis: A case series, *PMR*, 2009;1:604-11.
- Sheffler LR, et al., Functional effect of an ankle foot orthosis on gait in multiple sclerosis: A pilot study, *Am J Phys Med Rehabil*, 2008;87:26-32.
- Kim CM, et al., Effects of a simple functional electric system and/or a hinged ankle-foot orthosis on walking in persons with incomplete spinal cord injury, *Arch Phys Med Rehabil*, 2004;85:1718-23.
- Kottink AI, et al., The orthotic effect of functional electrical stimulation on the improvement of walking in stroke patients with a dropped foot: A systematic review, *Artif Organs*, 2004;28:577-86.
- Laufer Y, et al., Gait in individuals with chronic hemiparesis, *J Neurol Phys Ther*, 2009;33:104-10.
- Daly JJ, Response of gait deficits to neuromuscular electrical stimulation for stroke survivors, *Expert Rev Neurotherapeutics*, 2006;6:1511-22.
- Esnouf JE, et al., Impact on activities of daily living using a functional electrical stimulation device to improve dropped foot in people with multiple sclerosis, measured by the Canadian occupational performance measure, *Multiple Sclerosis*, 2010;16:1141-7.
- Barrett CL, et al., A randomized trial to investigate the effects of functional electrical stimulation and therapeutic exercise on walking performance for people with multiple sclerosis, *Mult Scler*, 2009;15:493-504.
- Paul L, et al., The effect of functional electrical stimulation on the physiological cost of gait in people with multiple sclerosis, *Mult Scler*, 2008;14:954-61.
- Ring H, Treger I, Gruendlinger L, Hausdorff JM, Neuroprosthesis for footdrop compared with an ankle-foot orthosis, *J Stroke Cerebrovasc Dis*, 2009;18:41-7.
- Bailey SN, et al., Neurotherapeutic and neuroprosthetic effects of implanted functional electrical stimulation for ambulation after incomplete spinal cord injury, *J Rehabil Res Dev*, 2010;47:7-16.
- Thrasher TA, et al., Gait training regimen for incomplete spinal cord injury using functional electrical stimulation, *Spinal Cord*, 2006;44:357-61.
- Field-Fote EC, Combined use of body weight support, functional electric stimulation, and treadmill training to improve walking ability in individuals with chronic incomplete spinal cord injury, *Arch Phys Med Rehabil*, 2001;82:818-24.
- Seifart A, et al., The effect of lower limb functional electrical stimulation on gait of children with cerebral palsy, *Pediatr Phys Ther*, 2009;21:23-30.
- van der Linden ML, et al., Functional electrical stimulation to the dorsiflexors and quadriceps in children with cerebral palsy, *Pediatr Phys Ther*, 2008;20:23-9.
- Everaert DG, et al., Does functional electrical stimulation for foot drop strengthen corticospinal connections?, *Neurorehabil Neural Repair*, 2010;24:168-77.
- Stein RB, et al., A multicenter trial of a footdrop stimulator controlled by a tilt sensor, *Neurorehabil Neural Repair*, 2006;20:371-9.
- Paul L, et al., The effect of functional electrical stimulation on the physiological cost of gait in people with multiple sclerosis, *Mult Scler*, 2008;14:954-61.
- Taylor PN, et al., Clinical use of the odstock dropped foot stimulator, *Arch Phys Med Rehabil*, 1999;80:1577-83.